



Normal haemodynamic parameters

Parameter	Equation	Normal range
Arterial Blood Pressure (BP)	Systolic (SBP) Diastolic (DBP)	90-140 mmHg 60-90 mmHg
Mean Arterial Pressure (MAP)	$[SBP + (2 \times DBP)]/3$	70-105 mmHg
Right Atrial Pressure (RAP) Central Venous Pressure (CVP)		2-6 mmHg (CVP normal range is equivalent to RAP)
Right Ventricular Pressure (RVP)	Systolic (RVSP) Diastolic (RVDP)	15-25 mmHg 0-8 mmHg
Pulmonary Artery Pressure (PAP)	Systolic (PASP) Diastolic (PADP)	15-25 mmHg 8-15 mmHg
Mean Pulmonary Artery Pressure (MPAP)	$[PASP + (2 \times PADP)]/3$	10-20 mmHg
Pulmonary Artery Occlusion Pressure (PAOP)		6-12 mmHg
Left Atrial Pressure (LAP)		6-12 mmHg
Cardiac Output (CO)	$HR \times SV/1000$	4-8 L/min
Cardiac Index (CI)	CO/BSA	2.5-4 L/min/m ²
Stroke Volume (SV)	$CO/HR \times 1000$	60-100 mL/beat
Stroke Volume Index (SVI)	$CI/HR \times 1000$	33-47 mL/m ² /beat
Stroke Volume Variation (SVV)	$100 \times (SV_{max} - SV_{min}) / \text{mean}(SV)$	<10-15%
Systemic Vascular Resistance (SVR)	$MAP - RAP \times 80 / CO$	800-1200 dynes/sec/cm ⁵
Systemic Vascular Resistance Index (SVRI)	$MAP - RAP \times 80 / CI$	1970-2390 dynes/sec/cm ⁵ /m ²
Pulmonary Vascular Resistance (PVR)	$MPAP - PAOP \times 80 / CO$	100-250 dynes/sec/cm ⁵
Pulmonary Vascular Resistance Index (PVRI)	$MPAP - PAOP \times 80 / CI$	255-285 dynes/sec/cm ⁵ /m ²



Additional haemodynamic parameters


Parameter	Equation	Normal range
Cardiac Power Index (CPI)	$MAP \times CI \times 0.0022$	0.5-0.7 W/m ²
Coronary Artery Perfusion Pressure (CPP)	Diastolic BP-PAOP	60-80 mmHg
Right Ventricular End-Diastolic Volume (RVEDV)	SV/EF	100-160 mL
Right Ventricular End-Diastolic Volume Index (RVEDVI)	RVEDV/1.7	59-94 mL/m ²
Right Ventricular End-Systolic Volume (RVESV)	EDV-SV	50-100 mL
Right Ventricular Ejection Fraction (RVEF)	SV/EDV	40-60%
Left Ventricular Stroke Work Index (LVSWI)	$SVI \times (MAP - PAOP) \times 0.0136$	50-62 g-m/m ² /beat
Right Ventricular Stroke Work Index (RVSWI)	$SVI \times (MPAP - RAP) \times 0.0136$	5-10 g-m/m ² /beat

Normal oxygenation parameters

Parameter	Equation	Normal range
Arterial Oxygen Saturation (SaO ₂)		95-100%
Mixed Venous Saturation (SvO ₂)		60-80%
Cerebral Tissue Oxygen Saturation (StO ₂)		60-80%
Arterial Oxygen Content (CaO ₂)	$(0.0138 \times Hb \times SaO_2) + (0.0031 \times PaO_2)$	17-20 mL/dL
Venous Oxygen Content (CvO ₂)	$(0.0138 \times Hb \times SvO_2) + (0.0031 \times PvO_2)$	12-15 mL/dL
A-V Oxygen Content Difference [C(a-v)O ₂]	CaO ₂ - CvO ₂	4-6 mL/dL
Oxygen Delivery (DO ₂)	CaO ₂ x CO x 10	950-1150 mL/min
Oxygen Delivery Index (DO ₂ I)	CaO ₂ x CI x 10	500-600 mL/min/m ²
Oxygen Consumption (VO ₂)	C(a-v)O ₂ x CO x 10	200-250 mL/min/m ²
Oxygen Consumption Index (VO ₂ I)	C(a-v)O ₂ x CI x 10	120-160 mL/min/m ²
Oxygen Extraction Ratio (O ₂ ER)	$[(CaO_2 - CvO_2) / CaO_2] \times 100$	22-30%
Oxygen Extraction Index (O ₂ EI)	$[(SaO_2 - SvO_2) / SaO_2] \times 100$	20-25%

Acumen HPI software parameters

- The HPI parameter displays as a value ranging from 0 to 100, with higher values indicating higher likelihood of hypotension
- The HPI value is updated every 20 seconds
- If the HPI parameter value exceeds 85, an auditory alarm will sound; if the HPI parameter exceeds 85 for two consecutive readings or reaches 100 at any time, the HPI high alert popup will appear, prompting you to review the patient haemodynamics using the HPI secondary screen

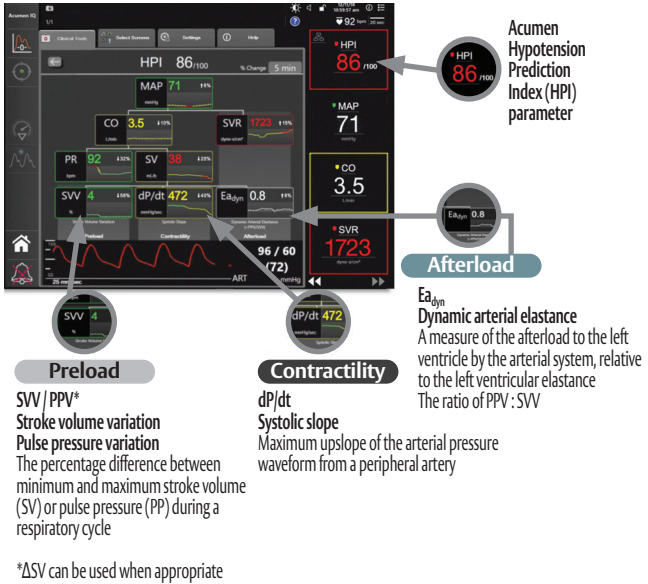

Normal blood laboratory values

Test	Convention units (reference values*)	SI units
Hematocrit (Hct)	Males: 41-50% Females: 35-45%	0.41-0.50 0.35-0.45
Hemoglobin (Hgb)	Males: 13.5-17.5 g/dL Females: 12.0-15.5 g/dL	135-175 g/L 120-155 g/L
Lactate	0.93-1.65 mEq/L	0.93-1.65 mmol/L

SI Units = International Units

*Reference Values vary by regional laboratory techniques and methods.

Edwards Clinical Education (ECE)

Experience our comprehensive education tools



ECE website



ECE YouTube



Acumen HPI software learning portal

For professional use. For a listing of indications, contraindications, precautions, warnings, and potential adverse events, please refer to the Instructions for Use (consult eifu.edwards.com where applicable).

Edwards devices placed on the European market meeting the essential requirements referred to in Article 3 of the Medical Device Directive 93/42/EEC bear the CE marking of conformity.

Edwards, Edwards Lifesciences, the stylized E logo, Acumen, Hypotension Prediction Index, HPI, and HemoSphere are trademarks of Edwards Lifesciences Corporation. All other trademarks are the property of their respective owners.

© 2022 Edwards Lifesciences Corporation.
All rights reserved. PP--EU-4269 v1.0

Edwards Lifesciences • edwards.com
Route de l'Etraz 70, 1260 Nyon, Switzerland



Edwards